



File D:\DATA

Injection Date : 6 Mar 15 7:37 pm +0800 Tgt Mass(EZX) :
Sample Name : 533 Location : P1-A-09
Acq. Operator : LCMS Inj : 1
Spec. Reported : MS Integration Inj Volume : 0.6 ul
Acq. Method : C:\CHEM32\1\METHODS\2-HPLC-15MIN.M
Analysis Method : C:\CHEM32\1\METHODS\2-HPLC-15MIN.M
Sample Info : *** No target masses specified ***
Method Info : Mobile Phase: A: water(0.01%TFA) B: ACN(0.01%TFA)
Gradient: 0min 5%B,3min 5%B,10min 95%B,15min 95%B
Flow Rate: 1.2 ml/min
Column: Eclipse XDB-C18,4.6*150mm,5um
Oven Temperature: 40 C


ADC1 A, ELSD

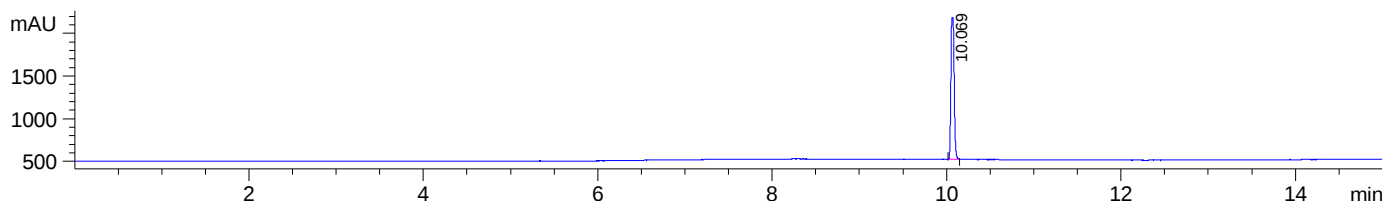


DAD1 A, Sig=214,4 Ref=off

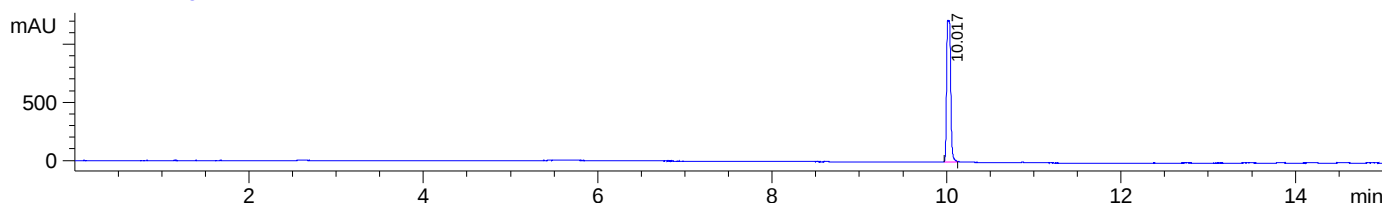

DAD1 B, Sig=254,4 Ref=off

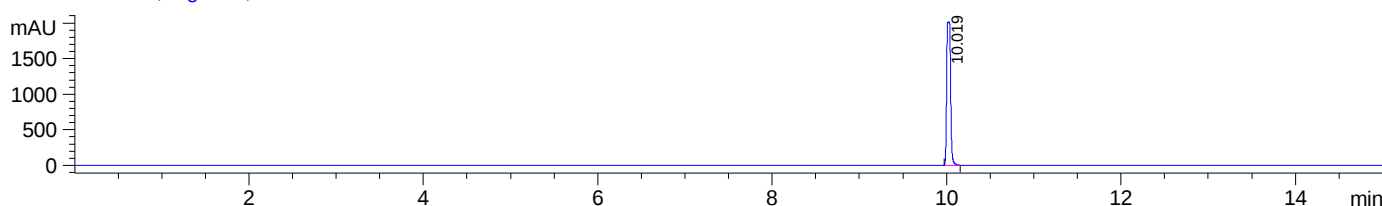

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70 **** NO MS PEAKS INTEGRATED ****

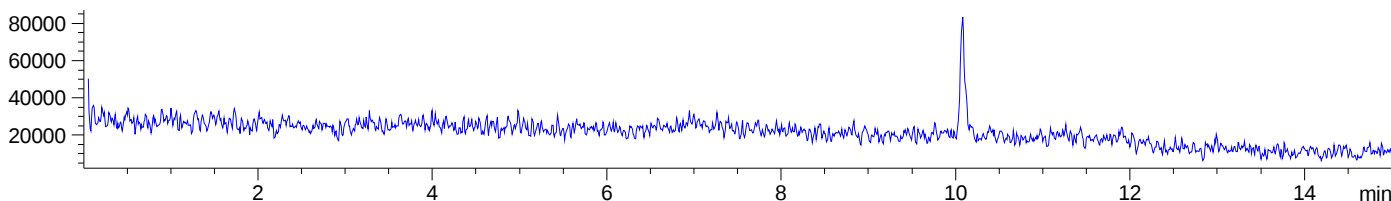

Integration Results for ADC1 A, ELSD

RetTim	Width	Area	Height	Area%
10.07	0.04	4293.48	1661.88	100.00

Integration Results for DAD1 A, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%
10.02	0.04	3911.27	1225.83	100.00

Integration Results for DAD1 B, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%
10.02	0.04	6252.70	2018.27	100.00